


Reprocessing Steps

This document outlines key components that must be included during each stage of reprocessing in order to achieve disinfection or sterilization of medical equipment/devices in community health care settings. For more information visit www.publichealthontario.ca or email ipac@oahpp.ca.

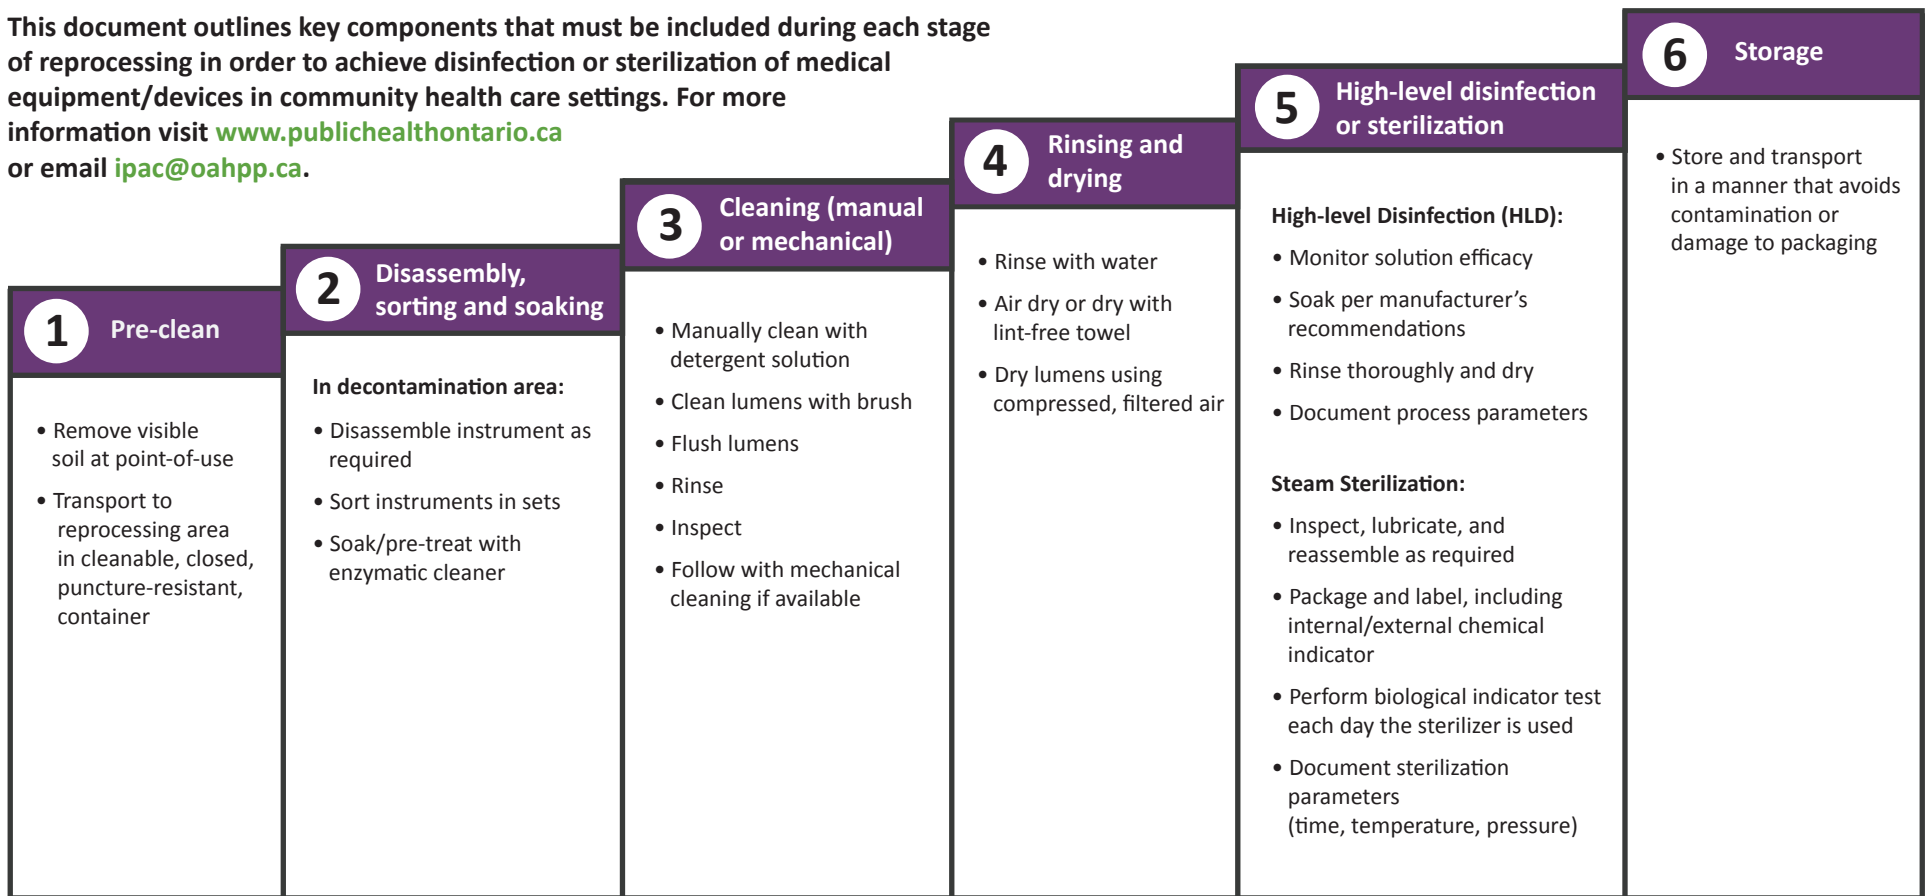

Reference:

Ontario Agency for Health Protection and Promotion (Public Health Ontario), Provincial Infectious Diseases Advisory Committee. Best practices for cleaning, disinfection and sterilization in all health care settings. 3rd ed. Toronto, ON: Queen's Printer for Ontario; 2013. Available from: http://www.publichealthontario.ca/en/eRepository/PIDAC_Cleaning_Disinfection_and_Sterilization_2013.pdf

CSA Group. Z314.3-14 Effective sterilization in health care facilities by the steam process. Mississauga, ON: CSA Group; 2014